

<https://doi.org/10.24875/RECICE.M20000156>

New technique for the emergent repositioning of the displaced Impella device



Nueva técnica para la recolocación emergente del Impella desplazado

Jorge García-Carreño,^{a,b} Teresa Bastante,^{b,c} Enrique Gutiérrez-Ibañes,^{a,b,d,*} María Eugenia Vázquez,^{a,b} Fernando Alfonso,^{b,c} and Francisco Fernández-Avilés^{a,b,e}

^a Servicio de Cardiología, Hospital General Universitario Gregorio Marañón, Madrid, Spain

^b Centro de Investigación Biomédica en Red de Enfermedades Cardiovasculares (CIBERCV), Spain

^c Servicio de Cardiología, Hospital Universitario de La Princesa, Universidad Autónoma de Madrid, Madrid, Spain

^d Departamento de Ingeniería Biomédica y Aeroespacial, Universidad Carlos III, Madrid, Spain

^e Facultad de Medicina, Universidad Complutense de Madrid, Madrid, Spain

To the Editor,

The use of circulatory support has grown exponentially over the last decade, particularly for the management of cardiogenic shock in the setting of acute myocardial infarction.^{1,2} The devices more often used like the Impella CP (Abiomed, United States) show good results in observational studies. These studies describe an improved survival rate when these devices are used as part of a well-defined program to treat cardiogenic shock.³⁻⁵ However, this is not a risk-free therapy, and device displacement is a complication that can occur while the patient is being moved or transferred. Although rare, this complication can be deadly if not solved immediately because there is a loss of hemodynamic support. In these cases, the device needs to be retrieved due to the impossibility of crossing the aortic valve to proceed with a new implant.

We present a new technique for the emergent percutaneous repositioning of the Impella CP device as performed in 3 cases in 2 different hospitals. Informed consent was obtained from the patients or their relatives for the publication of their cases.

The complete displacement of the Impella CP device towards the aorta poses several technical difficulties regarding repositioning. In the first place, it is not easy to cross the aortic valve with the device just by pushing it; what will probably happen is that it will crash into 1 of the leaflets running the risk of damaging them. Secondly, it cannot be mounted over a conventional 0.035 in guidewire, only over a special 0.018 in guidewire, that happens to be unavailable in the cath lab. Also, it needs to be inserted through a guidewire that runs across the Impella CP device motor and can be retrieved after implantation, which is why a correct reinsertion is very difficult to achieve, if not impossible. Lastly, if the 14-Fr introducer sheath has been removed, as it is usually the case to extract and reinsert the Impella CP device, the artery needs to be recanalized with a new introducer sheath. For all these reasons, the way to reverse the Impella CP displacement is usually to replace it completely with the corresponding delay and high cost.

The reinsertion technique presented here consists of facilitating the aortic valve crossing through an easy maneuver that keeps it open for a few seconds. Using the radial access and a 0.035 in guidewire a 5-Fr/6-Fr pigtail catheter is advanced towards the left ventricle and pushed until it spins around the ventricle to eventually exit through the aortic valve. The guidewire should be kept inside the catheter for further support. This in-and-out loop keeps the valve open, which allows an easy advance of the Impella CP device until its correct positioning ([figure 1](#)); this last maneuver should be performed carefully to avoid vascular complications. If it encounters any sort of resistance in the valvular plane, it is pulled back just a few centimeters and a new attempt is made with a small rotation. In 1 of the cases reported the valve could not be crossed during the first attempt and in the other 2 cases, 3 or 4 attempts were needed. However, the valve was always crossed in a few minutes and without immediate complications ([video 1 of the supplementary data](#)). Although significant aortic regurgitation almost surely occurs while performing the maneuver, it was well tolerated in all cases, probably due to its short duration and added benefit of restoring circulatory support.

From December 2015 through December 2019, 97 Impella CP devices were implanted in our hospitals. In 7 of them (7.2%) catheter displacement was reported. In 3 of the cases, the displacement was limited to the outflow tract and repositioned at the intensive care unit. In the remaining 4 cases, the displacement was total, the catheter was retrieved from the left ventricle all the way to the aorta and hemodynamic support was lost. In 1 of these patients, support was being withdrawn, which is why the device was eventually removed. The remaining 3 required the emergent repositioning of the device using the technique described here. [Table 1](#) shows the characteristics of these patients. The procedure was successful and without complications, and circulatory support was immediately recovered in the 3 cases. However, due to these patients' critical condition, 2 of them died a few days later of irreversible multiple organ failure.

* **Corresponding author:** Servicio de Cardiología, Hospital General Universitario Gregorio Marañón, Dr. Esquerdo 46, 28007 Madrid, Spain.
E-mail address: egutibanes@gmail.com [E. Gutiérrez-Ibañes].

Online: 21-09-2020.

2604-7322 / © 2020 Sociedad Española de Cardiología. Published by Permanyer Publications. This is an open access journal under the CC BY-NC-ND 4.0 license.

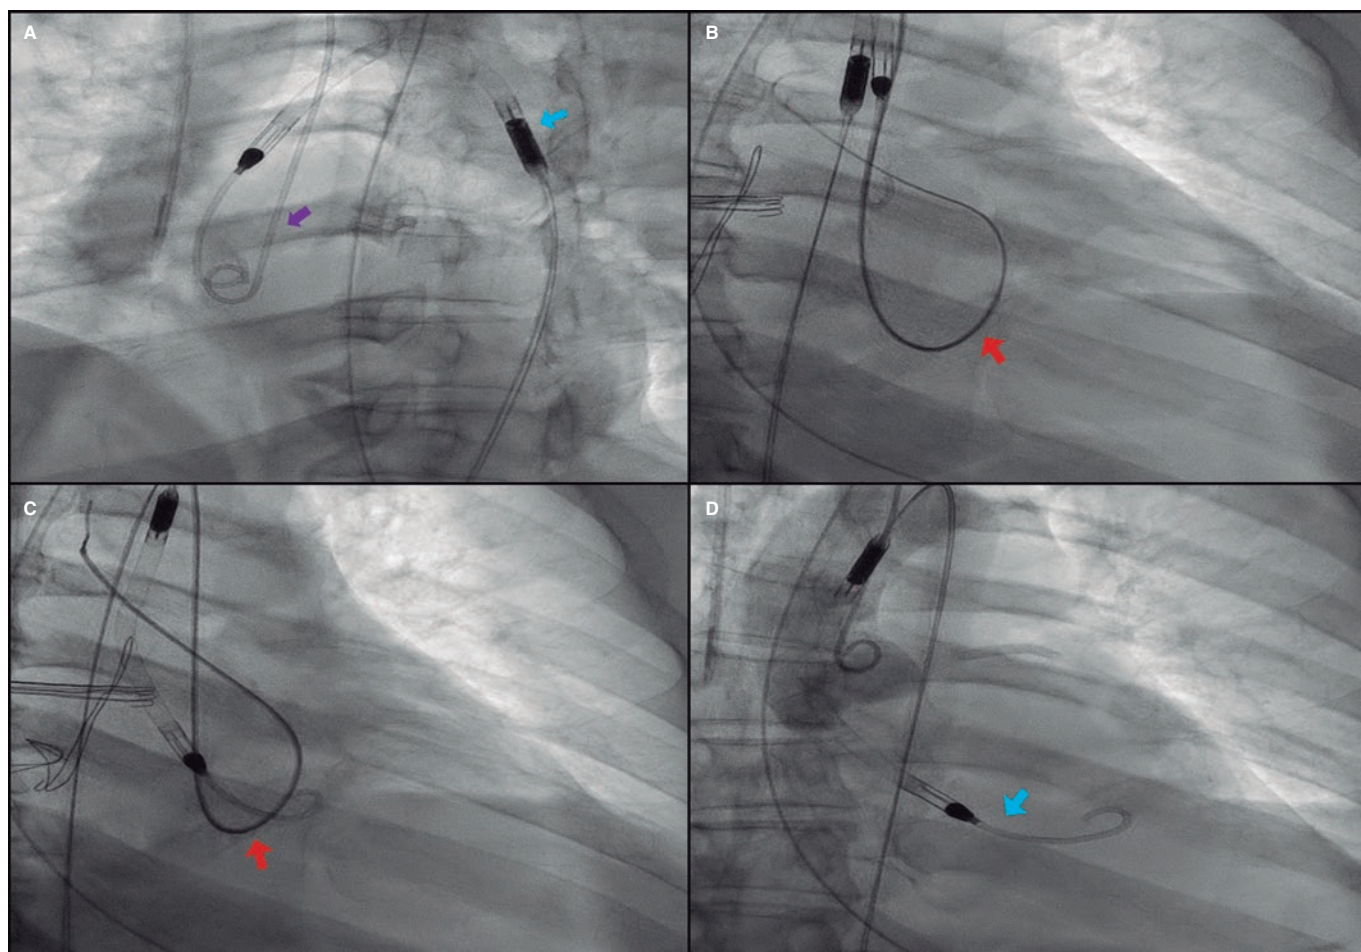


Figure 1. Impella CP device repositioning technique. **A:** pigtail catheter insertion (purple arrow) via radial access. Note how the Impella CP catheter has been displaced towards the ascending aorta (blue arrow). **B:** formation of intraventricular loop with the pigtail catheter keeping the 0.035 in guidewire to improve circulatory support (red arrow) while running across the aortic annulus, which facilitates its exit towards the aorta and keeps the valve open. **C:** afterwards, the Impella CP catheter (red arrow) is carefully advanced and pulled back by performing small rotations, if necessary, until reaching its final position (**D**, blue arrow).

Table 1. Characteristics of patients in whom the Impella CP device was repositioned

	Case #1	Case #2	Case #3
Age (years)	66	75	46
Sex	Male	Male	Male
Reason for the implant	Cardiogenic shock in the AMI setting	Electrical storm	LV unloading (APE after ECMO)
Previous LVEF (%)	20	20	5-10
Previous lactate (mmol/L)	5.1	4.2	> 15
Vasoactive drugs	NA + DBT	NA	NA + DBT
Additional support	ECMO	ECMO	ECMO
Impella access	Left femoral access	Right femoral access	Right femoral access
Cause of displacement	Transfer of the patient	Mobilization during x-ray	Accidental removal at the operating room
Successful repositioning	Yes	Yes	Yes
Hemodynamic improvement	Yes	Yes	Yes
Survival	No	No	Yes (transplant)

AMI, acute myocardial infarction; APE, acute pulmonary edema; DBT, dobutamine; ECMO, extracorporeal membrane oxygenation; LV, left ventricle; LVEF, left ventricular ejection fraction; NA, noradrenaline.

In conclusion, we presented a safe, efficient, cost-effective, and rapid technique that could be widely used to solve the Impella CP device displacement, minimize its potential consequences, and reduce costs.

FUNDING

No funding has been received.

AUTHORS' CONTRIBUTION

M.E. Vázquez, T. Bastante, and E. Gutiérrez-Ibañes conducted the procedures. J. García-Carreño and E. Gutiérrez-Ibañes wrote the article. M.E. Vázquez, T. Bastante, F. Fernández-Avilés and F. Alfonso supervised and corrected the article.

CONFLICTS OF INTEREST

F. Alfonso is associate editor of REC: Interventional Cardiology. The journal's editorial procedure to ensure impartial handling of the manuscript has been followed.

SUPPLEMENTARY DATA



Supplementary data associated with this article can be found in the online version available at <https://doi.org/10.24875/RECICE.M20000156>.

REFERENCES

1. Berg D, Barnett C, Kenigsberg B, et al. Clinical Practice Patterns in Temporary Mechanical Circulatory Support for Shock in the Critical Care Cardiology Trials Network (CCCTN) Registry. *Circ Heart Fail.* 2019;12: e006635.
2. Amin AP, Spertus JA, Curtis JP, et al. The Evolving Landscape of Impella® Use in the United States Among Patients Undergoing Percutaneous Coronary Intervention with Mechanical Circulatory Support. *Circ.* 2020;141: 273-284.
3. Basir MB, Kapur NK, Patel K, et al. Improved Outcomes Associated with the use of Shock Protocols: Updates from the National Cardiogenic Shock Initiative. *Catheter Cardiovasc Interv.* 2019;93:1173-1183.
4. Basir MB, Schreiber T, Dixon S, et al. Feasibility of early mechanical circulatory support in acute myocardial infarction complicated by cardiogenic shock: The Detroit cardiogenic shock initiative. *Catheter Cardiovasc Interv.* 2018;91:454-461.
5. Tehrani B, Truesdell A, Singh R, Murphy C, Saulino P. Implementation of a Cardiogenic Shock Team and Clinical Outcomes (INOVA-SHOCK Registry): Observational and Retrospective Study. *JMIR Res Protoc.* 2018;7:e160.

<https://doi.org/10.24875/RECICE.M20000162>

Percutaneous closure of aortic pseudoaneurysm

Cierre percutáneo de pseudoaneurisma aórtico

Francisco Pomar Domingo,^{a,*} Margarita Gudin Uriel,^a Alba López March,^b Miguel Jerez Valero,^b and Enrique Peris Domingo^a

^a Servicio de Cardiología, Hospital Universitario de La Ribera, Alzira, Valencia, Spain

^b Servicio de Cardiología, Hospital Manises, Manises, Valencia, Spain

To the Editor,

Aortic pseudoaneurysm is a rare high-risk complication following surgery with aortic manipulation.

This is the case of a 66-year-old male patient with a past medical history of aortic valve replacement 16 years ago. He required a second surgery 3 months later due to prosthetic valve endocarditis with mechanical valve replacement with homograft valve implantation. Since then, the patient has remained asymptomatic until 1 year ago when he developed progressive dyspnea. The echocardiographic study revealed severe aortic regurgitation with heavily calcified valve and ascending aorta. A new surgical intervention was performed to replace the homograft by a bioprosthesis. Surgery was very complex due to the presence of significant calcification. Two months after this last intervention the patient was admitted with clinical signs of thoracic pain and hemoptysis. The computed tomography scan performed revealed the presence of a narrow-necked aortic pseudoaneurysm at the ascending aorta lateral wall,

probably at the level of the cannulation performed during the previous surgery with a large periaortic hematoma (figure 1). Although the surgical repairment of the aortic pseudoaneurysm is the routine treatment, in this case it would have been the fourth reintervention. Instead, percutaneous treatment was decided.

Numerous articles have been published, most on isolated clinical cases, describing the closure of an aortic pseudoaneurysm with occluder devices different to the ones often used for the closure of septal defects, vascular plugs, etc. or coil embolization.^{1,2} No comparative studies have ever been conducted on the different treatment options available. We only found an article in the medical literature published by Lyen et al.³ that described a combined strategy in 7 patients with coil release and implantation of an occluder device in the same procedure. We also found a simple strategy with occluder device implantation in 5 patients with better results compared to the combined strategy. In our case, since the aortic pseudoaneurysm was large and the entry neck was small, a stepped combined strategy was decided of coil embolization and if



* Corresponding author: Unidad de Cardiología Intervencionista, Hospital Universitario de La Ribera, Ctra. Corbera km 1, 46600 Alzira, Valencia, Spain. E-mail address: pomar_fra@gva.es (F. Pomar Domingo).

Online: 06-11-2020.

2604-7322 / © 2020 Sociedad Española de Cardiología. Published by Permanyer Publications. This is an open access journal under the CC BY-NC-ND 4.0 license.